

Status report

07/05/2019


Tokyo University of Science

Michitaka Inomoto

Normal PMT

- We measured the dark rate of a normal PMT with negative HV.
- We checked difference in the dark rate with a normal PMT and a HA coated PMT.

Normal PMT

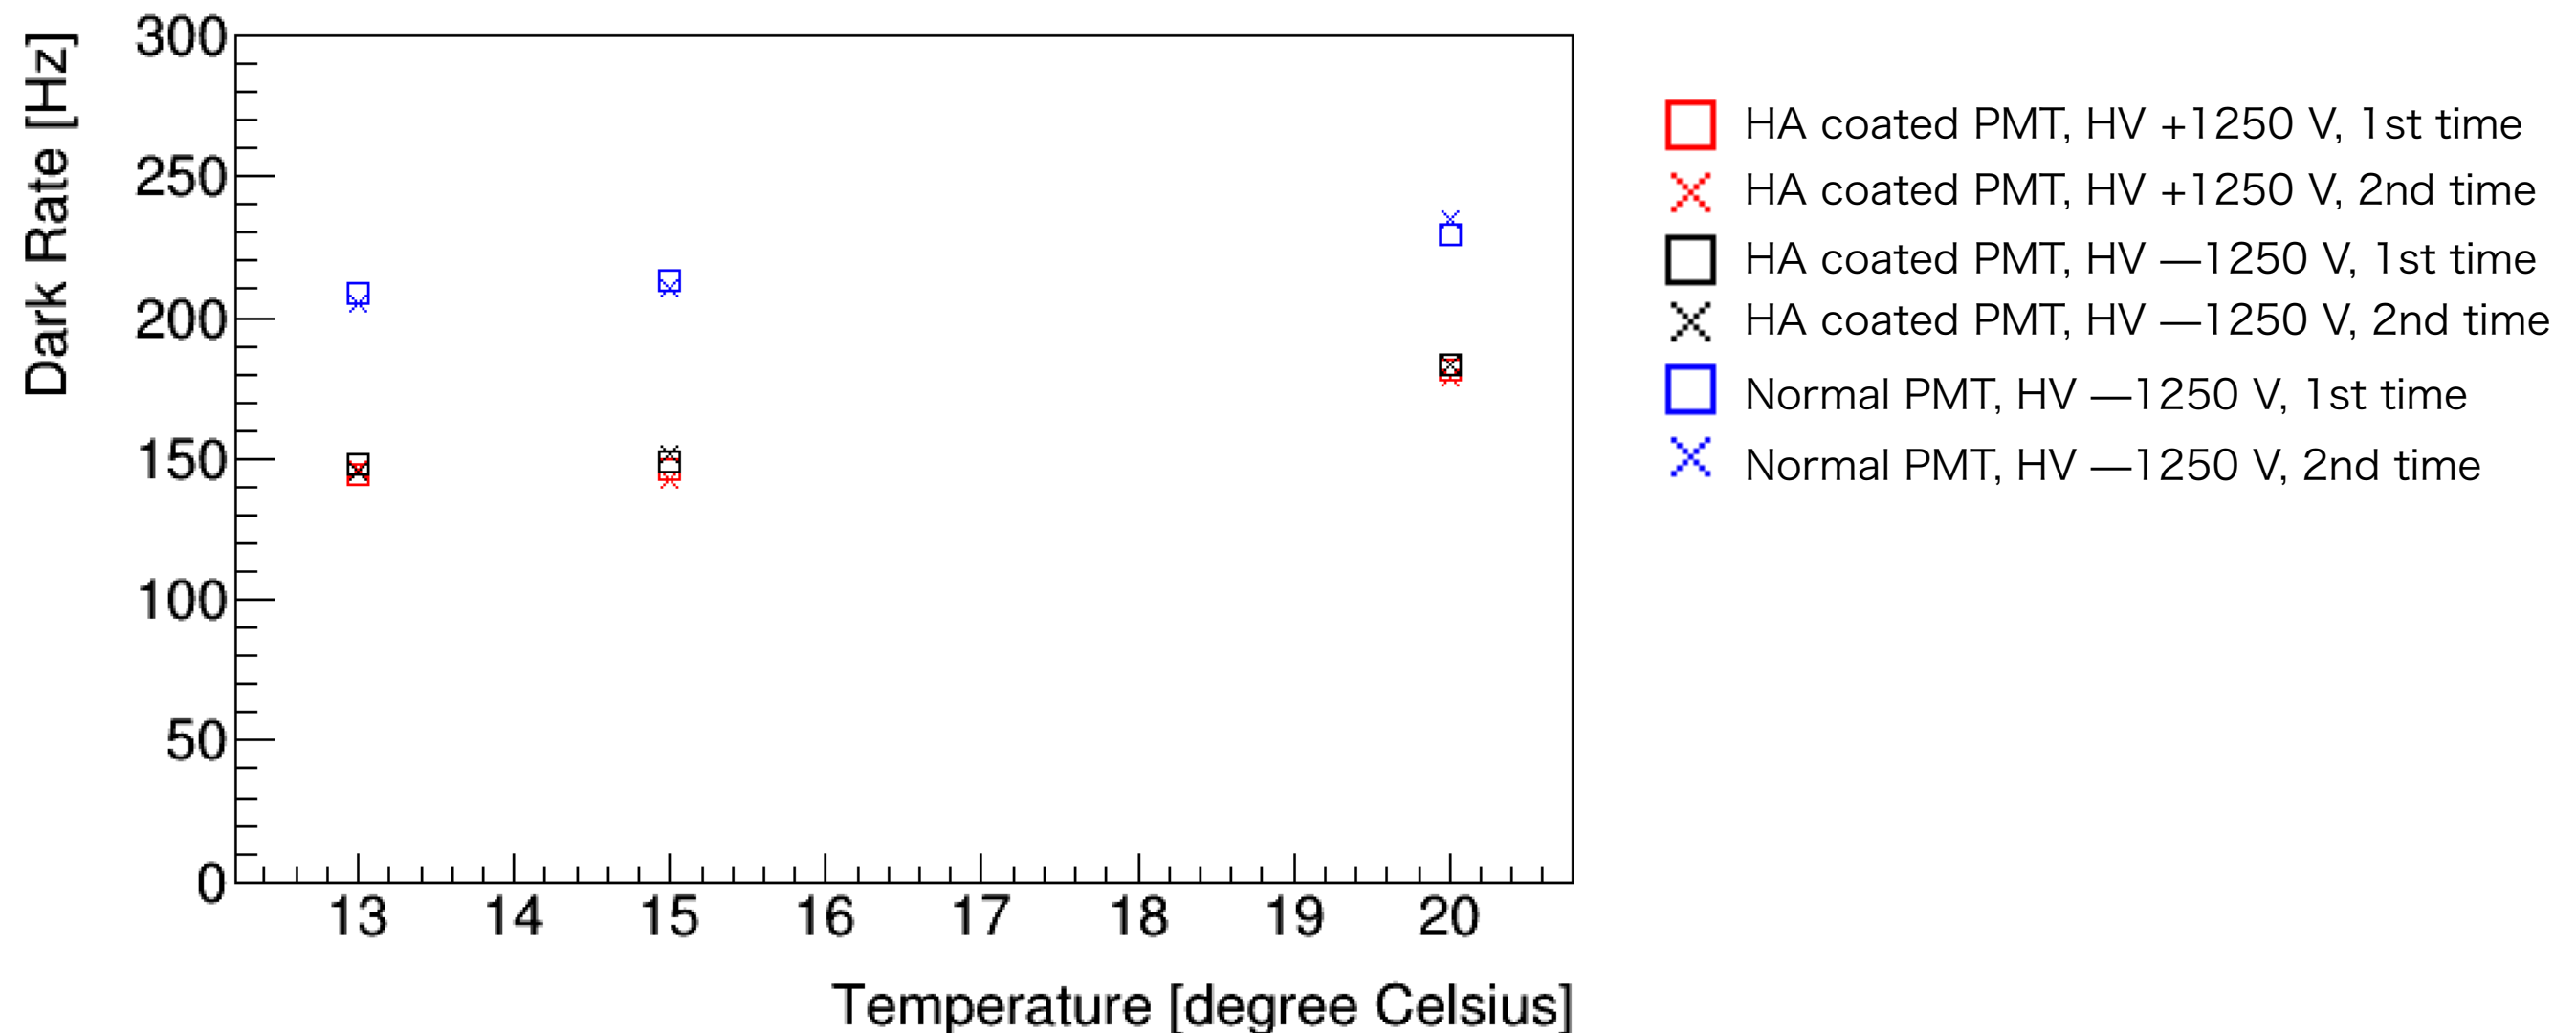

- The dark rate of a normal PMT with negative HV is higher than that of a HA coated PMT.

Future plan

- We will measure the dark rate of the normal PMT with positive HV.
- We will measure the dark rate of another normal PMT with negative HV and positive HV.